

メタクリル酸 = 2,3 エポキシプロピルのラットを用いた  
吸入によるがん原性試験報告書

試験番号 : 0794

# APPENDICES

## APPENDICES

- APPENDIX 1-1 IDENTITY OF 2,3-EPOXYPROPYL METHACRYLATE IN THE 2-YEAR INHALATION STUDY
- APPENDIX 1-2 STABILITY OF 2,3-EPOXYPROPYL METHACRYLATE IN THE 2-YEAR INHALATION STUDY
- APPENDIX 2 ENVIRONMENTAL CONDITIONS OF INHALATION CHAMBER IN THE 2-YEAR INHALATION STUDY OF 2,3-EPOXYPROPYL METHACRYLATE
- APPENDIX 3 METHODS, UNITS AND DECIMAL PLACE FOR HEMATOLOGY AND BIOCHEMISTRY IN THE 2-YEAR INHALATION STUDY OF 2,3-EPOXYPROPYL METHACRYLATE

APPENDIX 1-1

IDENTITY OF 2,3-EPOXYPROPYL METHACRYLATE  
IN THE 2-YEAR INHALATION STUDY

IDENTITY OF 2,3-EPOXYPROPYL METHACRYLATE IN THE 2-YEAR INHALATION STUDY

Test Substance : 2,3-Epoxypropyl methacrylate (SIGMA-ALDRICH)

A. Lot No. : MKBF2342V



1. Spectral Data

Mass Spectrometry

Instrument : Hitachi M-80B Mass Spectrometer

Ionization : EI (Electron Ionization)

Ionization Voltage : 70eV

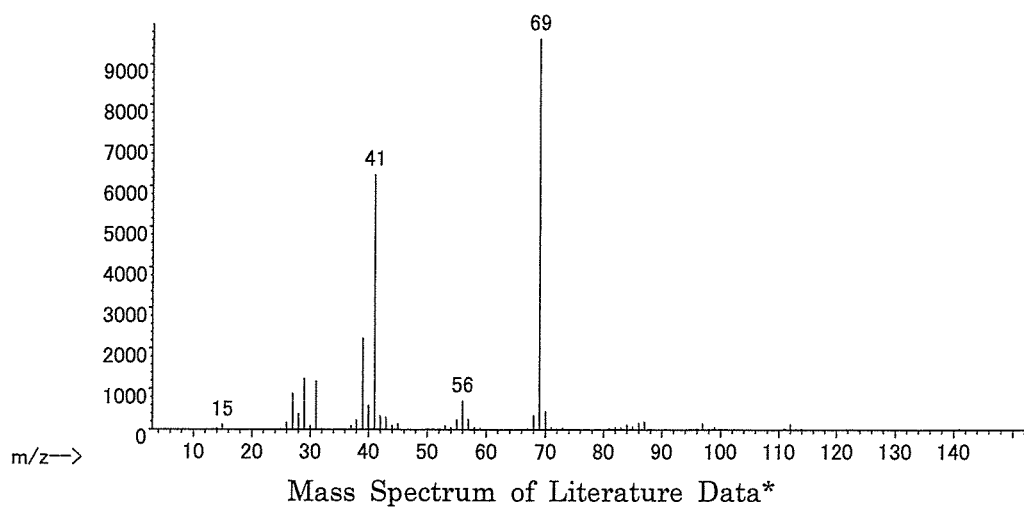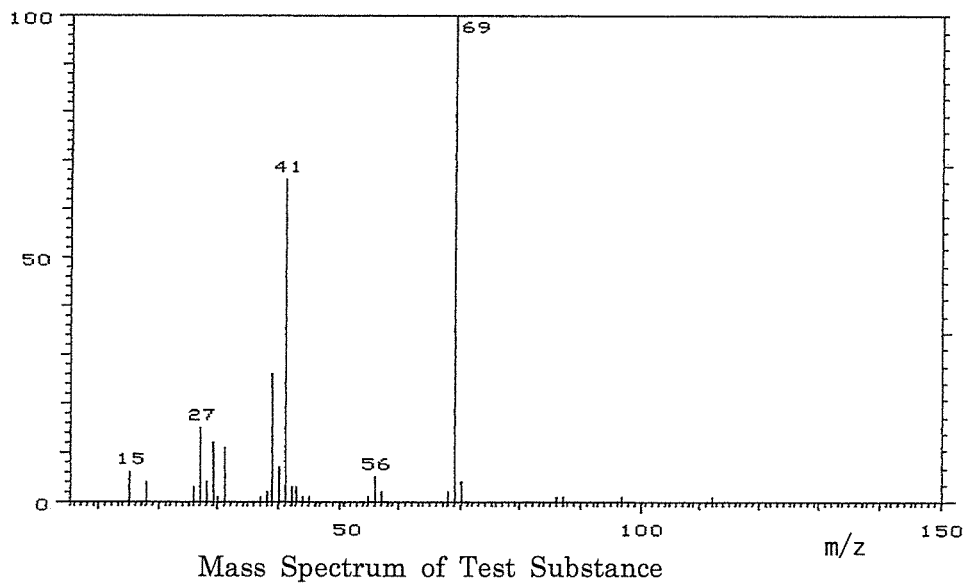

Result: The mass spectrum was consistent with literature spectrum.


(\*McLafferty FW, ed. 1994. Wiley Registry of Mass Spectral Data. 6th ed. New York, NY:John Wiley and Sons.)

Infrared Spectrometry


Instrument : Shimadzu FTIR-8200PC Infrared Spectrometer

Cell : KBr Liquid Cell

Resolution : 4 cm<sup>-1</sup>

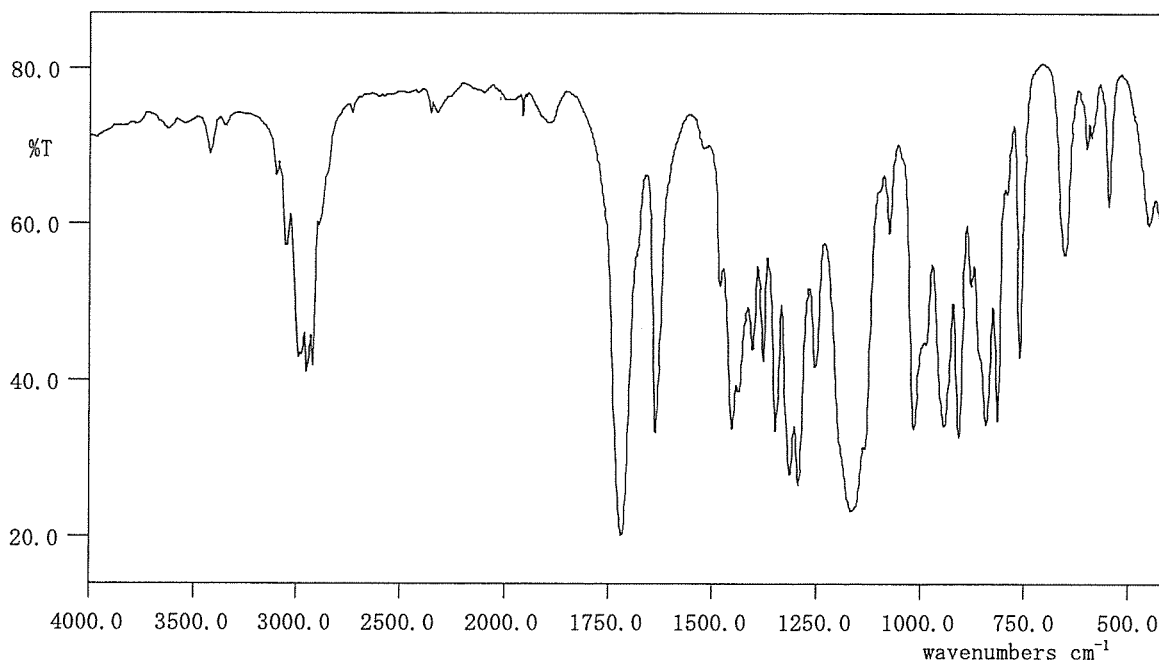

Infrared Spectrum of Test Substance

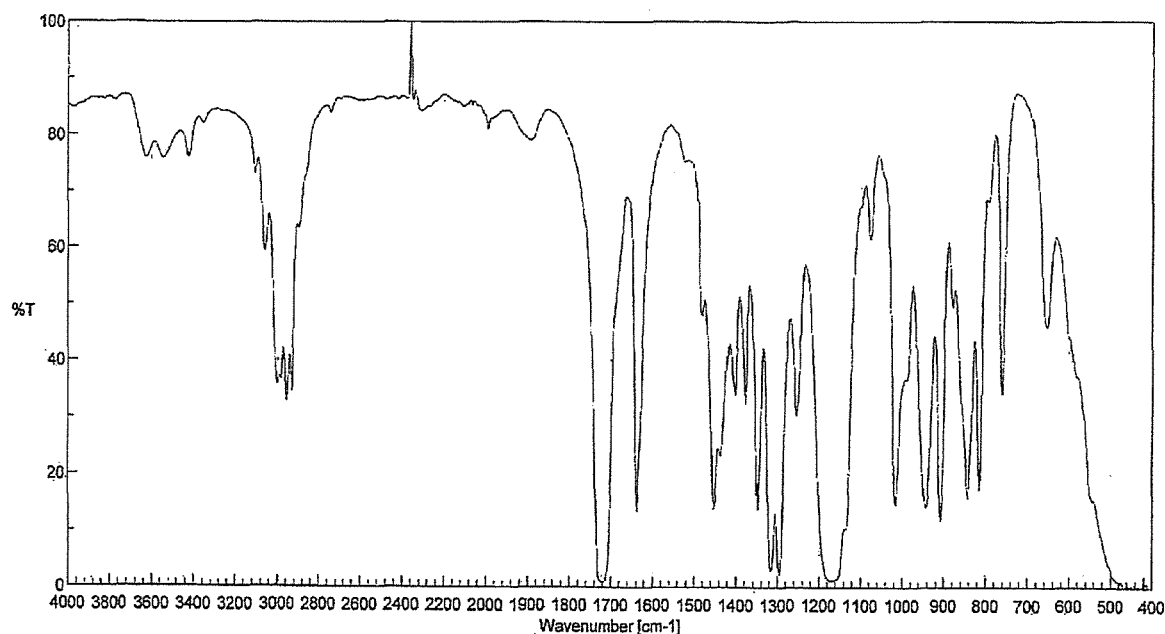

Infrared Spectrum of Literature Data\*

Result: The infrared spectrum was consistent with literature spectrum.

(\*Performed by Wako Pure Chemical Industries, Ltd.)

2. Conclusion: The test substance was identified as 2,3-epoxypropyl methacrylate by mass spectrum and infrared spectrum.

B. Lot No. : MKBG6062V



1. Spectral Data

Mass Spectrometry

Instrument : Hitachi M-80B Mass Spectrometer

Ionization : EI (Electron Ionization)

Ionization Voltage : 70eV

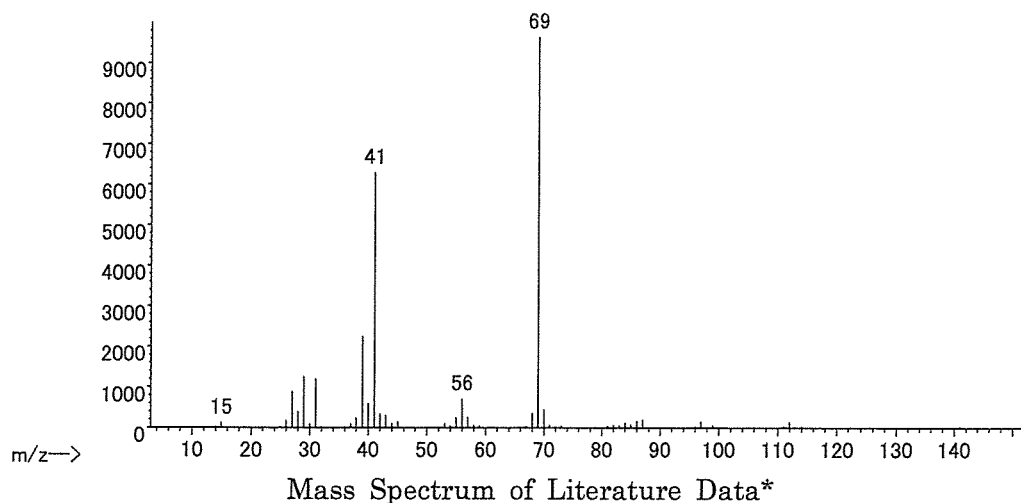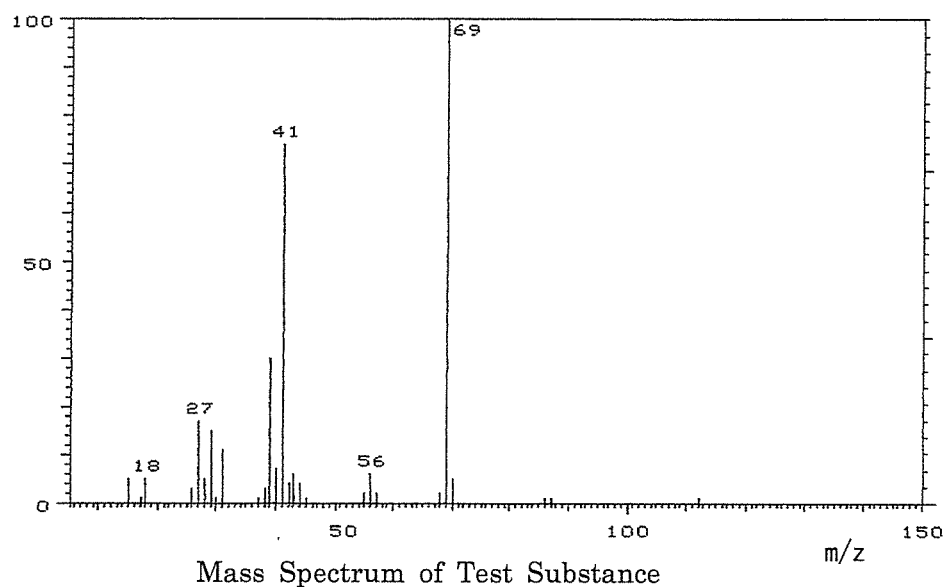


Result: The mass spectrum was consistent with literature spectrum.

(\*McLafferty FW, ed. 1994. Wiley Registry of Mass Spectral Data. 6th ed. New York, NY:John Wiley and Sons.)


Infrared Spectrometry

Instrument : Shimadzu FTIR-8200PC Infrared Spectrometer

Cell : KBr Liquid Cell

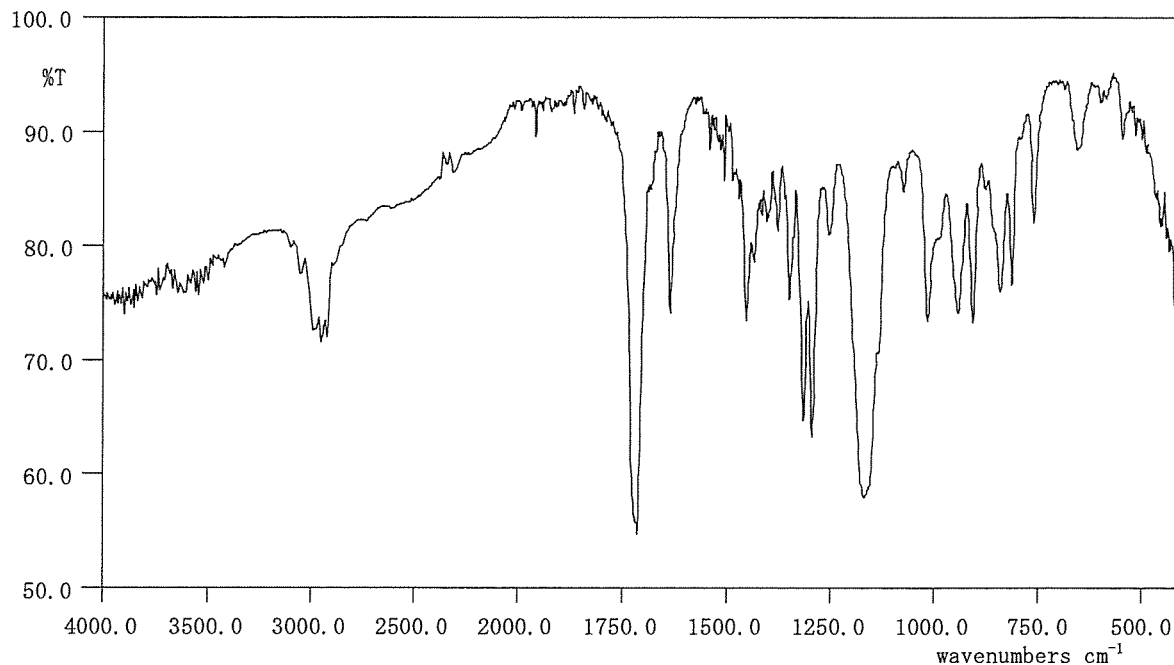Resolution : 4  $\text{cm}^{-1}$ 

Infrared Spectrum of Test Substance

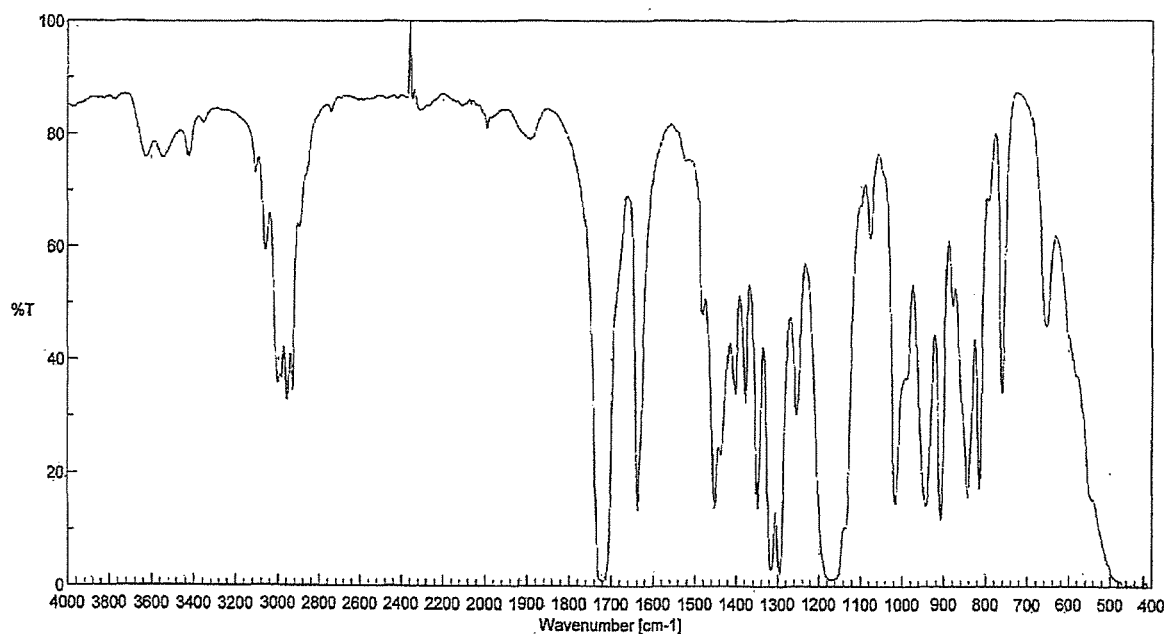

Infrared Spectrum of Literature Data\*

Result: The infrared spectrum was consistent with literature spectrum.

(\*Performed by Wako Pure Chemical Industries, Ltd.)

2. Conclusion: The test substance was identified as 2,3-epoxypropyl methacrylate by mass spectrum and infrared spectrum.

C. Lot No. : MKBH2577V



1. Spectral Data

Mass Spectrometry

Instrument : Hitachi M-80B Mass Spectrometer

Ionization : EI (Electron Ionization)

Ionization Voltage : 70eV

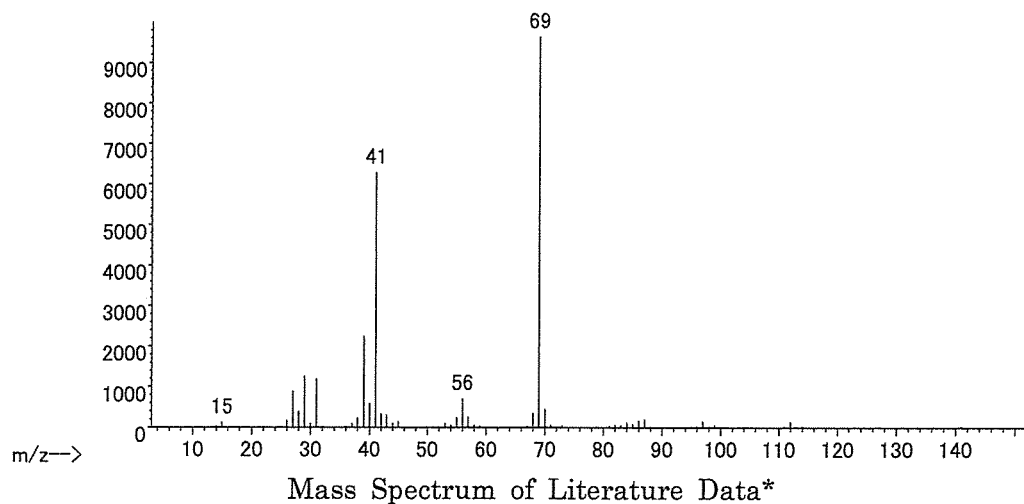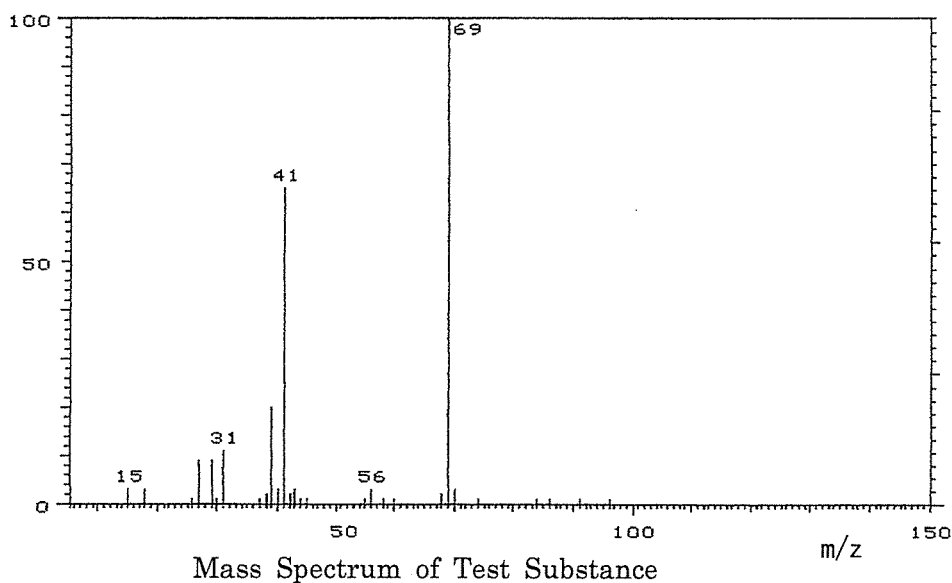

Result: The mass spectrum was consistent with literature spectrum.  
(\*McLafferty FW, ed. 1994. Wiley Registry of Mass Spectral Data. 6th ed.  
New York, NY:John Wiley and Sons.)




Infrared Spectrometry


Instrument : Shimadzu FTIR-8200PC Infrared Spectrometer

Cell : KBr Liquid Cell

Resolution : 4  $\text{cm}^{-1}$

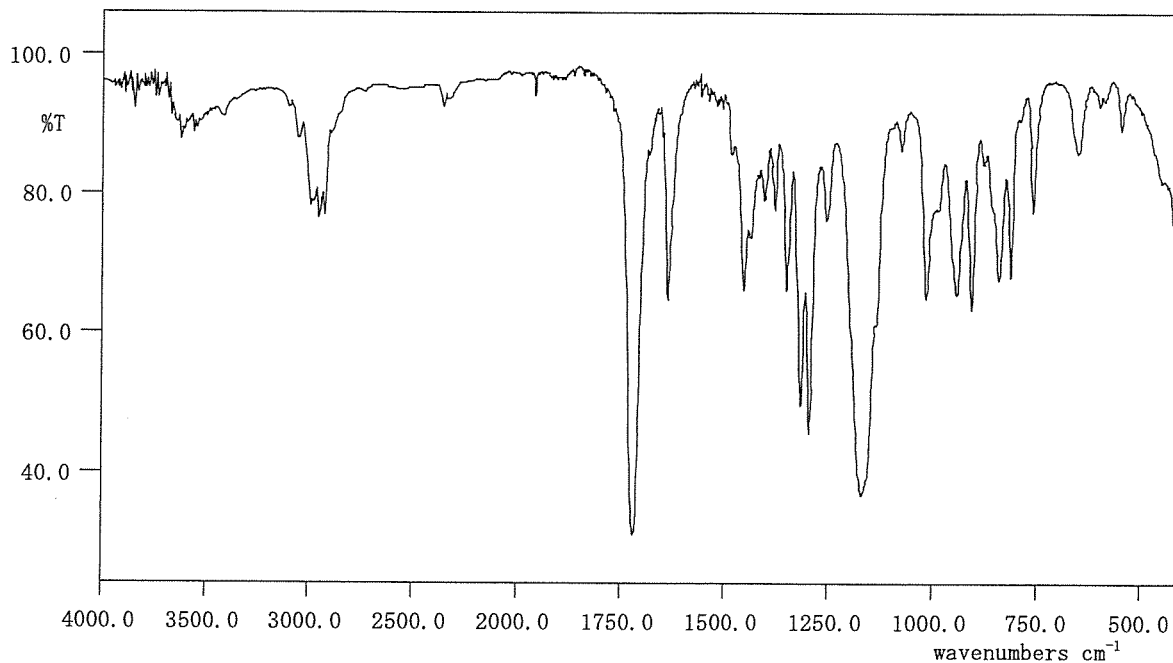

Infrared Spectrum of Test Substance

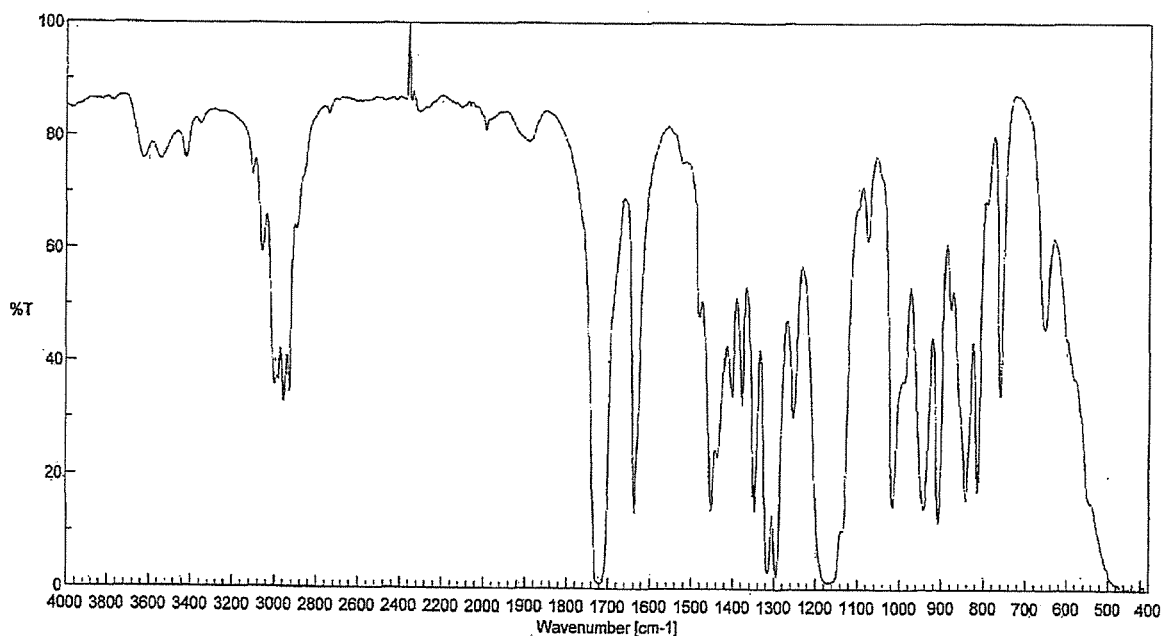

Infrared Spectrum of Literature Data\*

Result: The infrared spectrum was consistent with literature spectrum.

(\*Performed by Wako Pure Chemical Industries, Ltd.)

2. Conclusion: The test substance was identified as 2,3-epoxypropyl methacrylate by mass spectrum and infrared spectrum.

APPENDIX 1-2

STABILITY OF 2,3-EPOXYPROPYL METHACRYLATE  
IN THE 2-YEAR INHALATION STUDY

## STABILITY OF 2,3-EPOXYPROPYL METHACRYLATE IN THE 2-YEAR INHALATION STUDY

Test Substance : 2,3-Epoxypropyl methacrylate (SIGMA-ALDRICH)

A. Lot No. : MKBF2342V

## 1. Gas Chromatography

Instrument : Agilent Technologies 5890A Gas Chromatograph

Column : Methyl Silicone (0.53 mm  $\phi$   $\times$  60 m)

Column Temperature : 180° C

Flow Rate : 10 mL/min

Detector : FID (Flame Ionization Detector)

Injection Volume : 1  $\mu$ L

Date (date analyzed)	Peak No.	Retention Time (min)	Area (%)
2012.01.27	1	3.792	100
2012.08.07	1	3.785	100

Result: Gas chromatography indicated one major peak (peak No. 1) analyzed on 2012.1.27 and one major peak (peak No. 1) analyzed on 2012.8.7. No new trace impurity peak in the test substance analyzed on 2012.8.7 was detected.

2. Conclusion: The test substance was stable for the period that the test substance had been used for the study.

B. Lot No. : MKBG6062V

1. Gas Chromatography

Instrument : Agilent Technologies 5890A Gas Chromatograph

Column : Methyl Silicone (0.53 mm  $\phi$   $\times$  60 m)

Column Temperature : 180° C

Flow Rate : 10 mL/min

Detector : FID (Flame Ionization Detector)

Injection Volume : 1  $\mu$ L

Date (date analyzed)	Peak No.	Retention Time (min)	Area (%)
2012.08.03	1	3.786	100
2013.08.02	1	3.830	100

Result: Gas chromatography indicated one major peak (peak No. 1) analyzed on 2012.8.3 and one major peak (peak No. 1) analyzed on 2013.8.2. No new trace impurity peak in the test substance analyzed on 2013.8.2 was detected.

2. Conclusion: The test substance was stable for the period that the test substance had been used for the study.

C. Lot No. : MKBH2577V

1. Gas Chromatography

Instrument : Agilent Technologies 5890A Gas Chromatograph

Column : Methyl Silicone (0.53 mm  $\phi$   $\times$  60 m)

Column Temperature : 180° C

Flow Rate : 10 mL/min

Detector : FID (Flame Ionization Detector)

Injection Volume : 1  $\mu$ L

Date (date analyzed)	Peak No.	Retention Time (min)	Area (%)
2013.07.29	1	3.821	100
2014.03.06	1	3.815	100

Result: Gas chromatography indicated one major peak (peak No. 1) analyzed on 2013.7.29 and one major peak (peak No. 1) analyzed on 2014.3.6. No new trace impurity peak in the test substance analyzed on 2014.3.6 was detected.

2. Conclusion: The test substance was stable for the period that the test substance had been used for the study.

## APPENDIX 2

# ENVIRONMENTAL CONDITIONS OF INHALATION CHAMBER IN THE 2-YEAR INHALATION STUDY OF 2,3-EPOXYPROPYL METHACRYLATE

ENVIRONMENTAL CONDITIONS OF INHALATION CHAMBER IN THE 2-YEAR  
INHALATION STUDY OF 2,3-EPOXYPROPYL METHACRYLATE

Group Name	Temperature (°C) Mean ± S.D.	Humidity (%) Mean ± S.D.	Ventilation Rate (L/min) Mean ± S.D.	Air Change (time/h) Mean
Control	23.1 ± 0.2	53.6 ± 1.5	1514.8 ± 9.7	12.0
3.2 ppm	23.1 ± 0.2	53.5 ± 2.2	1516.7 ± 8.8	12.0
8 ppm	23.1 ± 0.2	50.6 ± 2.5	1517.1 ± 9.8	12.0
20 ppm	23.1 ± 0.2	51.8 ± 2.6	1520.3 ± 9.2	12.0

## APPENDIX 3

METHODS, UNITS AND DECIMAL PLACE FOR  
HEMATOLOGY AND BIOCHEMISTRY  
IN THE 2-YEAR INHALATION STUDY OF  
2,3-EPOXYPROPYL METHACRYLATE



METHODS, UNITS AND DECIMAL PLACE FOR HEMATOLOGY AND BIOCHEMISTRY  
IN THE 2-YEAR INHALATION STUDY OF 2,3-EPOXYPROPYL METHACRYLATE

Item	Method	Unit	Decimal place
<b>Hematology</b>			
Red blood cell (RBC)	Light scattering method <sup>1)</sup>	$\times 10^6/\mu\text{L}$	2
Hemoglobin(Hgb)	Cyanmethemoglobin method <sup>1)</sup>	g/dL	1
Hematocrit(Hct)	Calculated as $\text{RBC} \times \text{MCV}/10$ <sup>1)</sup>	%	1
Mean corpuscular volume(MCV)	Light scattering method <sup>1)</sup>	fL	1
Mean corpuscular hemoglobin(MCH)	Calculated as $\text{Hgb}/\text{RBC} \times 10$ <sup>1)</sup>	pg	1
Mean corpuscular hemoglobin concentration (MCHC)	Calculated as $\text{Hgb}/\text{Hct} \times 100$ <sup>1)</sup>	g/dL	1
Platelet	Light scattering method <sup>1)</sup>	$\times 10^3/\mu\text{L}$	0
Reticulocyte	Light scattering method <sup>1)</sup>	%	1
White blood cell(WBC)	Light scattering method <sup>1)</sup>	$\times 10^3/\mu\text{L}$	2
Differential WBC	Light scattering method <sup>1)</sup>	%	0
<b>Biochemistry</b>			
Total protein(TP)	Biuret method <sup>2)</sup>	g/dL	1
Albumin (Alb)	BCG method <sup>2)</sup>	g/dL	1
A/G ratio	Calculated as $\text{Alb}/(\text{TP} - \text{Alb})$ <sup>2)</sup>	—	1
T-bilirubin	BOD method <sup>2)</sup>	mg/dL	2
Glucose	GlcK·G-6-PDH method <sup>2)</sup>	mg/dL	0
T-cholesterol	CE·COD·POD method <sup>2)</sup>	mg/dL	0
Triglyceride	MGLP·GK·GPO·POD method <sup>2)</sup>	mg/dL	0
Phospholipid	PLD·ChOD·POD method <sup>2)</sup>	mg/dL	0
Aspartate aminotransferase (AST)	JSCC method <sup>2)</sup>	U/L	0
Alanine aminotransferase (ALT)	JSCC method <sup>2)</sup>	U/L	0
Lactate dehydrogenase (LDH)	JSCC method <sup>2)</sup>	U/L	0
Alkaline phosphatase (ALP)	JSCC method <sup>2)</sup>	U/L	0
$\gamma$ -Glutamyl transpeptidase ( $\gamma$ -GTP)	JSCC method <sup>2)</sup>	U/L	1
Creatine kinase (CK)	JSCC method <sup>2)</sup>	U/L	0
Urea nitrogen	Urease·GLDH method <sup>2)</sup>	mg/dL	1
Creatinine	Creatinase·SOD·POD method <sup>2)</sup>	mg/dL	2
Sodium	Ion selective electrode method <sup>2)</sup>	mEq/L	0
Potassium	Ion selective electrode method <sup>2)</sup>	mEq/L	1
Chloride	Ion selective electrode method <sup>2)</sup>	mEq/L	0
Calcium	OCPC method <sup>2)</sup>	mg/dL	1
Inorganic phosphorus	PNP·XOD·POD method <sup>2)</sup>	mg/dL	1

1) Automatic blood cell analyzer (ADVIA120 : Siemens Healthcare Diagnostics Inc.)

2) Automatic analyzer (Hitachi 7080 : Hitachi,Ltd.)